

AD-A279 339



Factors That Determine Visual Acuity Through Night Vision Goggles for Emmetropes

By

John C. Kotulak

and

Stephen E. Morse

DTIC
ELECTE
MAY 18 1994
S G D

DTIC QUALITY INSPECTED 3

Aircrew Health and Performance Division

April 1994

Approved for public release; distribution unlimited.

94-14817

404 578

94 5 17 105

United States Army Aeromedical Research Laboratory
Fort Rucker, Alabama 36362-0577

Notice

Qualified requesters

Qualified requesters may obtain copies from the Defense Technical Information Center (DTIC), Cameron Station, Alexandria, Virginia 22314. Orders will be expedited if placed through the librarian or other person designated to request documents from DTIC.

Change of address

Organizations receiving reports from the U.S. Army Aeromedical Research Laboratory on automatic mailing lists should confirm correct address when corresponding about laboratory reports.

Disposition

Destroy this document when it is no longer needed. Do not return it to the originator.


Disclaimer

The views, opinions, and/or findings contained in this report are those of the author(s) and should not be construed as an official Department of the Army position, policy, or decision, unless so designated by other official documentation. Citation of trade names in this report does not constitute an official Department of the Army endorsement or approval of the use of such commercial items.


Human use


Human subjects participated in these studies after giving their free and informed voluntary consent. Investigators adhered to AR 70-25 and USAMRDC Reg 70-25 on Use of Volunteers in Research.

Reviewed:


RICHARD R. LEVINE
LTJG, MS
Director, Aircrew Health
and Performance Division

Released for publication:


ROGER W. WILEY, O.D., Ph.D.
Chairman, Scientific
Review Committee


DAVID H. KARNEY
Colonel, MC, SFS
Commanding

REPORT DOCUMENTATION PAGE				Form Approved OMB No. 0704-0188	
1a. REPORT SECURITY CLASSIFICATION Unclassified			1b. RESTRICTIVE MARKINGS		
2a. SECURITY CLASSIFICATION AUTHORITY			3. DISTRIBUTION / AVAILABILITY OF REPORT Public release; distribution unlimited		
2b. DECLASSIFICATION / DOWNGRADING SCHEDULE					
4. PERFORMING ORGANIZATION REPORT NUMBER(S) USAARL Report No. 94-16			5. MONITORING ORGANIZATION REPORT NUMBER(S)		
6a. NAME OF PERFORMING ORGANIZATION U.S. Army Aeromedical Research Laboratory		6b. OFFICE SYMBOL (If applicable) SGRD-UAB	7a. NAME OF MONITORING ORGANIZATION U.S. Army Medical Research and Development Command		
6c. ADDRESS (City, State, and ZIP Code) P.O. Box 620577 Fort Rucker, AL 36362-0577			7b. ADDRESS (City, State, and ZIP Code) Fort Detrick Frederick, MD 21702-5012		
8a. NAME OF FUNDING / SPONSORING ORGANIZATION		8b. OFFICE SYMBOL (If applicable)	9. PROCUREMENT INSTRUMENT IDENTIFICATION NUMBER		
8c. ADDRESS (City, State, and ZIP Code)			10. SOURCE OF FUNDING NUMBERS		
PROGRAM ELEMENT NO.		PROJECT NO.	TASK NO.		WORK UNIT ACCESSION NO.
0602787A		3M162 787879	BG		174
11. TITLE (Include Security Classification) (U) Factors that Determine Visual Acuity Through Night Vision Goggles for Emmetropes					
12. PERSONAL AUTHOR(S) John C. Kotulak and Stephen E. Morse					
13a. TYPE OF REPORT Final		13b. TIME COVERED FROM _____ TO _____		14. DATE OF REPORT (Year, Month, Day) 1994 April	
15. PAGE COUNT 19					
16. SUPPLEMENTARY NOTATION					
17. COSATI CODES			18. SUBJECT TERMS (Continue on reverse if necessary and identify by block number)		
FIELD	GROUP	SUB-GROUP	Night vision goggles, visual acuity, emmetropia, refractive error		
20	06				
23	02				
19. ABSTRACT (Continue on reverse if necessary and identify by block number) The purpose of this study was to investigate factors which could affect the visual acuity of emmetropes (individuals without clinically significant refractive error) while viewing through night vision goggles, namely unaided visual acuity, clinically insignificant refractive error, and experience as a visual observer. We found that night vision goggle visual acuity is related to unaided visual acuity for emmetropes when the night vision goggle eyepieces are focused to infinity, and that this relationship is robust with respect to changes in target contrast. We also found that both the unaided and night vision goggle (infinity focus eyepiece) visual acuity of nominal emmetropes is related to uncorrected refractive error, and that experience as a visual observer is significantly related to night vision goggle visual acuity. The implication of these results is that many aviators who are medically cleared to fly without glasses will suffer from reduced vision through any night vision device with a fixed infinity focus eyepiece. Similarly, ground vehicle operators who have astigmatism and who must use spectacle incompatible night vision goggles will also suffer from reduced visual acuity.					
20. DISTRIBUTION / AVAILABILITY OF ABSTRACT <input checked="" type="checkbox"/> UNCLASSIFIED/UNLIMITED <input type="checkbox"/> SAME AS RPT. <input type="checkbox"/> DTIC USERS			21. ABSTRACT SECURITY CLASSIFICATION Unclassified		
22a. NAME OF RESPONSIBLE INDIVIDUAL			22b. TELEPHONE (Include Area Code)		22c. OFFICE SYMBOL

Acknowledgments

The following personnel from the U.S. Army Aeromedical Research Laboratory are thanked for their contributions to this study: SPC Mark A. Kenzie, LTC James M. King, Dr. William E. McLean, LTC Jeffrey C. Rabin, Dr. Robert W. Verona, and Dr. Roger W. Wiley.

Accession For	
NTIS	CRA&I <input checked="checked" type="checkbox"/>
DTIC	TAB <input type="checkbox"/>
Unannounced <input type="checkbox"/>	
Justification	
By	
Distribution /	
Availability Codes	
Dist	Avail and/or Special
A-1	

This page intentionally left blank.

Table of contents

List of figures.....	2
List of tables.....	2
Introduction.....	3
Methods.....	5
Subjects.....	5
Apparatus.....	6
Procedures.....	7
Design and statistical analysis.....	7
Results.....	9
Bivariate relationships.....	9
Multivariate relationships.....	10
Fixed infinity focus aided visual acuity.....	11
Aided visual acuity for high contrast targets.....	11
Aided visual acuity for low contrast targets.....	14
User adjusted focus aided visual acuity.....	14
Discussion.....	14
References.....	17

List of figures

1. Relationship between resolving power of system components to that of the combined system.....	4
2. ANVIS modulation transfer function.....	4
3. Distribution of uncorrected unaided high contrast visual acuities.....	8
4. Distribution of uncorrected unaided low contrast visual acuities.....	8
5. Relationship between unaided visual acuity and astigmatism for nominal emmetropes.....	9
6. Relationship between aided visual acuity and sphere for nominal emmetropes.....	10
7. Relationship between aided and unaided acuity for emmetropes.....	11
8. Relationship between aided and unaided acuity comparing observed to predicted results.....	15

List of tables

1. Descriptive statistics of subjects.....	5
2. Target parameters.....	7
3. List of candidate independent variables to predict aided visual acuity (high contrast) when eyepiece is focused at infinity.....	12
4. List of candidate independent variables to predict aided visual acuity (low contrast) when the eyepiece is focused at infinity.....	12
5. List of candidate independent variables to predict aided visual acuity (high contrast) when the eyepiece is focused for best vision.....	13
6. List of candidate independent variables to predict aided visual acuity (low contrast) when the eyepiece is focused for best vision.....	13

Introduction

Many factors which could affect visual acuity (VA) with night vision goggles (NVGs) already have been studied, e.g., night sky condition and target contrast (Levine and Rash, 1989a and 1989b; Wiley, 1989; Kotulak and Rash, 1992), NVG generation (Miller et al., 1984; Kotulak and Rash, 1992), nuclear flashblindness protection (Levine and Rash, 1989a and 1989b), chemical protective masks (Miller et al., 1989; Donohue-Perry, Riegler, and Hausman, 1990), signal-to-noise ratio (Riegler et al., 1991), interpupillary distance misadjustment (King and Morse, 1992), and instrument myopia (Kotulak and Morse, 1992, 1994a, and 1994b; Kotulak, Morse, and Wiley, 1993). Another factor which could influence NVG VA is decreased unaided VA, i.e., VA without NVGs; however, relatively little is known about it.

Kim (1982) investigated the influence of astigmatism on NVG VA; however, he did not report the unaided VA of his subjects. Hoover (1983) measured both unaided and aided VA; however, most of Hoover's subjects suffered from vision loss due to eye disease. Therefore, it is not certain whether Hoover's results are relevant to healthy populations.

In the current report, we present measurements of both unaided and aided VA on healthy, emmetropic subjects in order to determine whether there is a correlation between the two. The theoretical basis for such an association comes from the following: When two optical systems of unequal resolving power are combined, the resolution of the combined system can be predicted by the equation below, in which R_H and R_L represent the resolving powers of the high and low resolution elements respectively, and R_C represents the resolving power of the combined system (Farrell and Booth, 1984).

$$\frac{1}{R_C^{1.7}} = \frac{1}{R_H^{1.7}} + \frac{1}{R_L^{1.7}}$$

An observer viewing through NVGs can be thought of as such a system, in which the eye is the high resolution element when the observer is emmetropic. Figure 1 is derived from the above equation by holding R_L constant at 20 cycles/degree (cpd), the approximate resolution limit of current NVGs (Figure 2), and varying R_H over a wide range. The equation predicts that the resolving power of the combined system is affected by changes in R_H , especially in the region at and below the eye's maximum resolution, which is approximately 40 cpd.

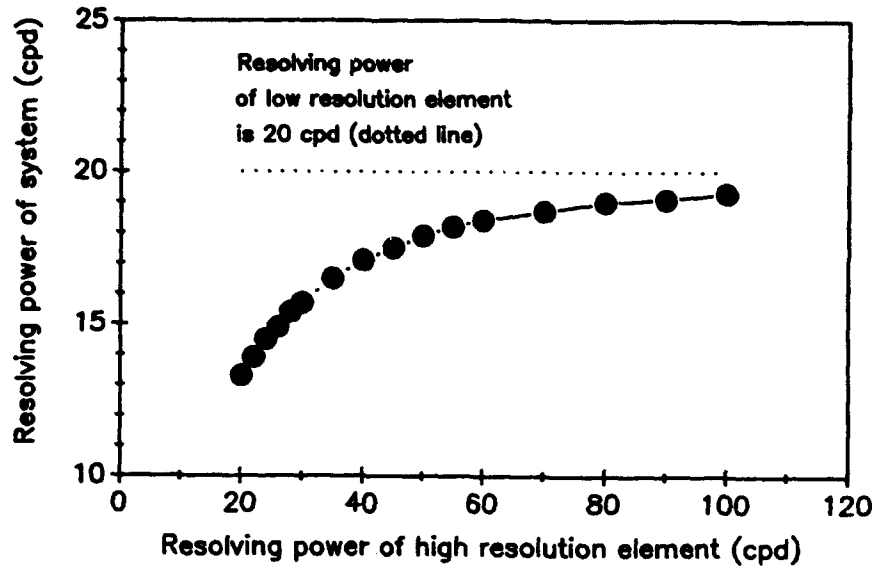


Figure 1. The relationship between the resolving power of the high resolution element and the combined system, given that the resolving power of the low resolution element is held constant. This model was derived from experiments with photographic systems (Farrell and Booth, 1984).

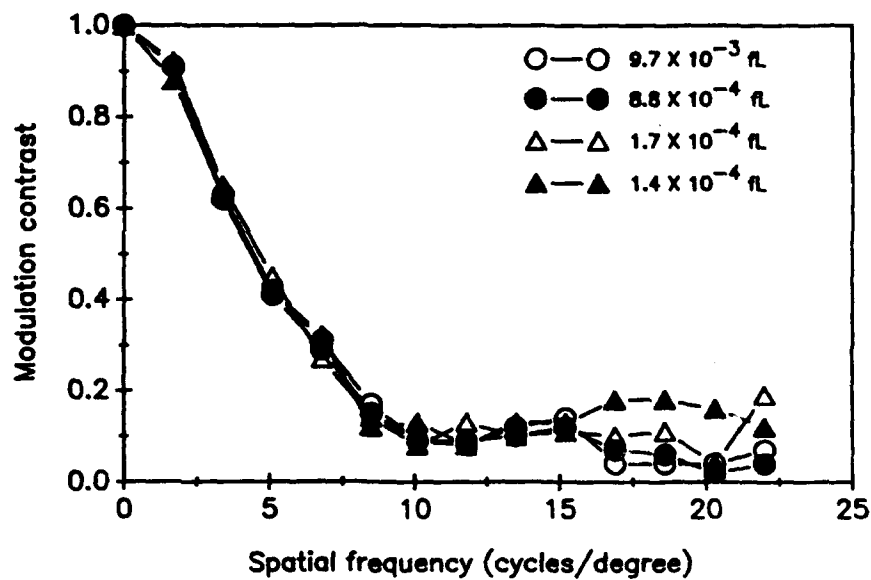


Figure 2. The ANVIS spatial modulation transfer function under varying levels of ambient luminance (Kotulak and Morse, 1994).

In this report, we also explore other factors which could influence NVG VA among emmetropes, namely refractive error and experience as a visual observer (flight experience and NVG experience). In the strictest sense, refractive error and emmetropia are mutually exclusive. However, emmetropes are commonly defined clinically as persons who have a distance VA of at least 20/20 in each eye, a condition which does not preclude small refractive errors (Hirsch, 1945).

Methods

Subjects

Sixteen volunteer subjects, who were either U.S. Army aviators ($n = 12$) or flight school students ($n = 4$), were recruited for the experiment. All subjects had unaided visual acuities of at least 20/20 in each eye, and were free from eye disease and other ocular anomalies. All of the subjects were cleared to fly without spectacles. Table 1 gives descriptive statistics regarding age, flight and NVG experience, and refractive error for the subjects. The refractive error data probably overestimate the degree of myopia by about 0.25 diopters (D) due to instrument myopia elicited by the autorefractor (Miwa, 1992).

Table 1.
Descriptive statistics of subjects.

Variable	Mean	SD	Median	Range
Age (years)	27.1	4.9	27.0	22 to 37
Total flight hours	988.1	1347.2	300.0	68 to 4000
Flight hours with NVGs	84.7	139.1	21.0	0 to 500
Equivalent sphere (D)	-0.35	0.37	-0.44	-0.88 to 0.50
Sphere (D)	-0.16	0.39	-0.25	-0.63 to 0.63
Cylinder (D)	-0.39	0.26	-0.25	-0.13 to -1.00

Apparatus

The NVG used in the study was the AN/AVS-6 Aviator Night Vision Imaging System (ANVIS) (Jenkins and Efkenan, 1980). ANVIS is a unity-magnification pair of binoculars which electronically amplify ambient light and thus provide photopic vision under night sky conditions. ANVIS consists of two identical monoculars, the main components of which are an objective, a third-generation image intensifier, and an eyepiece. The ANVIS modulation transfer function (Figure 2) demonstrates that the phosphor image is spatially lowpass filtered. As a result, VA with ANVIS under optimum conditions is only 20/35, and it gets worse with decreasing night sky luminance (Kotulak and Rash, 1992). The output luminance of ANVIS falls off steadily with decreases in input luminance when the latter is less than quarter moon, the lower limit of the ANVIS automatic gain control. This allows the ANVIS display luminance to be manipulated as an experimental variable.

The visual stimuli were high (Bailey and Lovie, 1976) and low (Bailey, 1982) contrast Bailey-Lovie acuity charts. Two versions of the chart, differing only in letter sequence, were used at each level of contrast. These charts were chosen because their scale is five times finer than that of Snellen-like charts, and their test-retest reliability is twice as great (Bailey et al., 1991). In addition, Bailey-Lovie charts incorporate an equal-interval scale that permits the use of parametric statistics (Lovie-Kitchin, 1988).

The contrast of the Bailey-Lovie optotypes was calculated from the equation below, in which L_B and L_L represent background and letter luminance respectively.

$$C = \frac{100(L_B - L_L)}{L_B}$$

Photometrically-measured luminance was used to calculate target contrast, both on the NVG phosphor screen under simulated night sky conditions (labelled "Aided" on Table 2), and on the charts themselves under photopic conditions (labelled "Unaided" on Table 2). Table 2 also gives the background luminance (i.e., the luminance of the white portion of the chart) for the aided and unaided conditions.

Table 2.
Target parameters.

Parameter	Aided		Unaided	
	High	Low	High	Low
Contrast (percent)	62	12	98	21
Luminance (cd/m ²)	6.5		6.5	

Procedures

VA always was measured under binocular conditions. The same charts were used for aided and unaided viewing. VA thresholds, which were defined as the common logarithm of the minimum angle of resolution {log MAR} (Bailey and Lovie, 1976), were recorded using Bailey-Lovie scoring procedures (Bailey and Lovie, 1976), without a time limit, and without reinforcement. Contrast changes were made by switching between charts. The order of presentation of the stimuli was randomized.

Prior to making focus adjustments, the subjects were trained to reach a most-plus endpoint, i.e., use the most plus (or least minus) dioptric power that was required for best vision. This is consistent with established clinical technique for refraction. Eyepiece power was verified with a dioptometer. Refractive error was measured objectively with an autorefractor.

Design and statistical analysis

The dependent variables were high and low contrast aided VA measured with the NVG eyepieces focused at infinity, and high and low contrast aided VA measured with the NVG eyepieces focused by the users for best vision. The design was within subjects. The correlation of the dependent variables with various candidate independent variables was tested by simple and multiple linear regression. The independent variables were high and low contrast unaided VA, total flight hours, NVG flight hours, and refractive error. Three refractive error components were considered separately, i.e., sphere, cylinder, and equivalent sphere (one-half the cylinder power plus the sphere power).

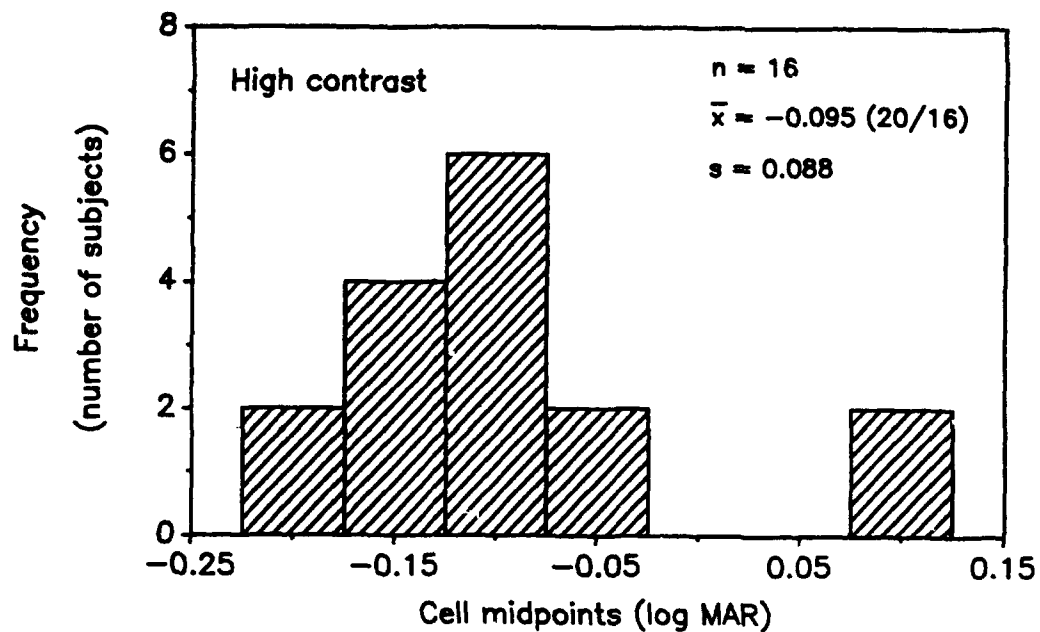


Figure 3. The distribution of uncorrected unaided visual acuities to high contrast letters for nominal emmetropes.

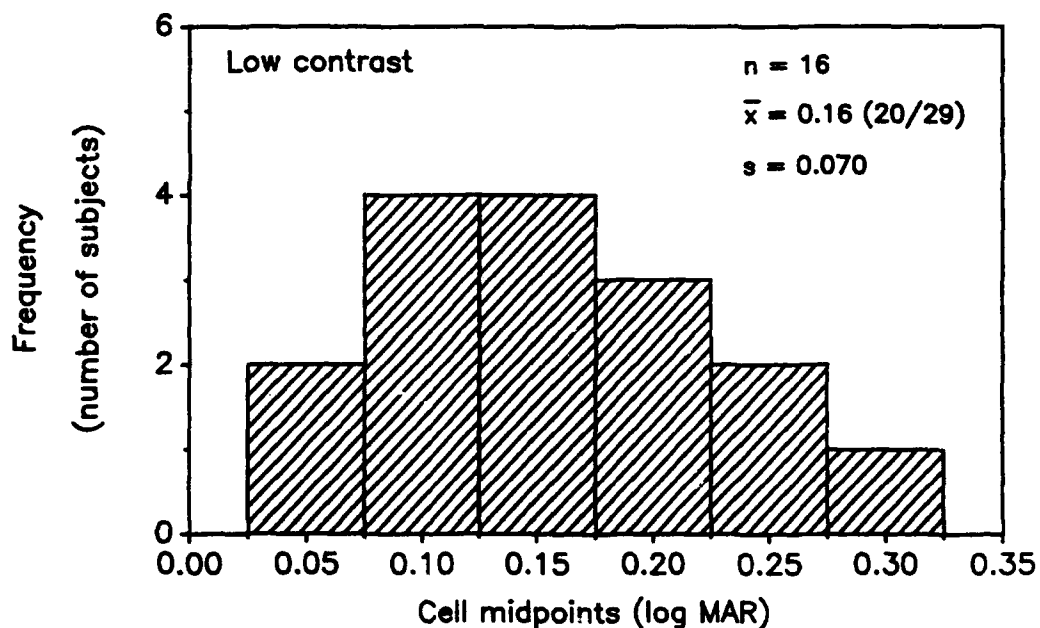


Figure 4. The distribution of uncorrected unaided visual acuities to low contrast letters for nominal emmetropes.

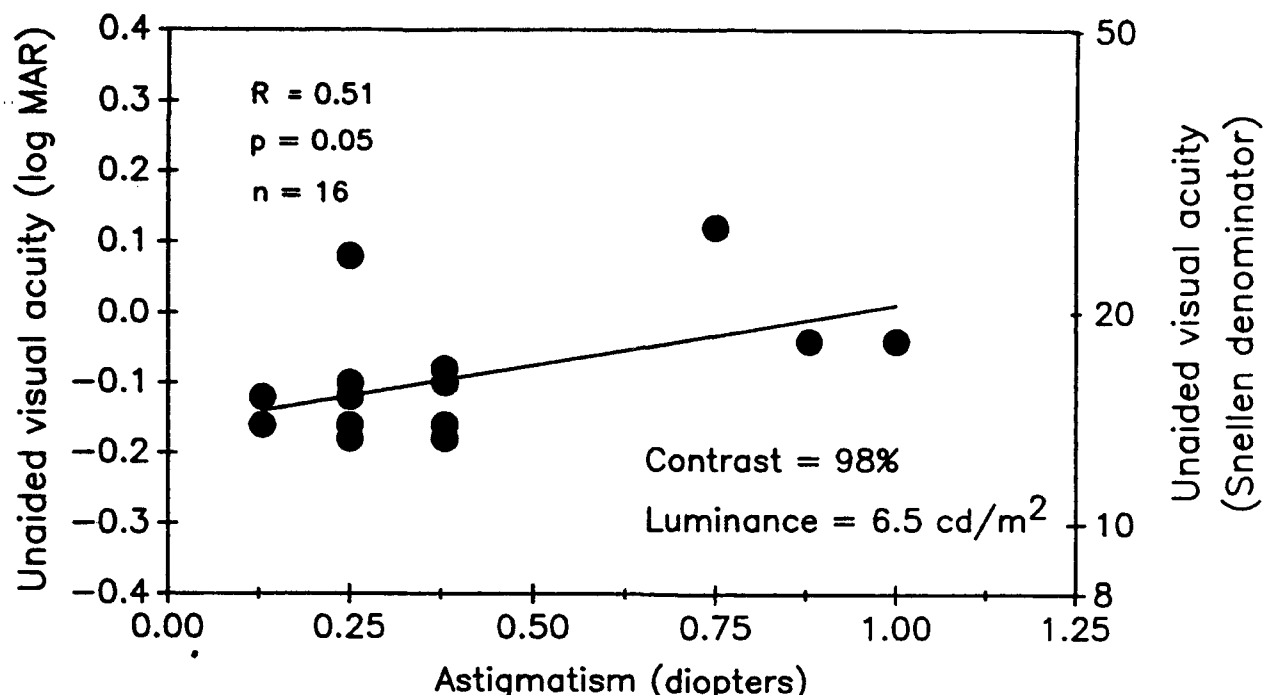


Figure 5. The relationship between uncorrected unaided VA and the absolute value of the astigmatic component of the refractive error for nominal emmetropes. The relatively low chart luminance, which was intended to match that of the NVG display, resulted in elevated acuity thresholds.

Results

Bivariate relationships

Figures 3 and 4 give the distributions of unaided VAs for our nominally emmetropic subjects at high and low target contrasts, respectively. Note that in Figure 3, two subjects had VAs less than 20/20. This was most likely due to the test luminance of 6.5 cd/m² (Sheedy, Bailey, and Raasch, 1984), which is considerably lower than the 85 cd/m² that is recommended for the clinical measurement of VA (National Research Council, 1979). The luminance of 6.5 cd/m² was selected because it matched the ANVIS display luminance (Table 2).

The variability in VA among emmetropes is due, at least partially, to uncorrected refractive error, as shown in Figure 5 (see also Table 1). Figure 5 demonstrates that unaided VA to high contrast letters is correlated with the amount of astigmatism. Similarly, the ANVIS VA of emmetropes also can be related to uncorrected refractive error. For example, Figure 6

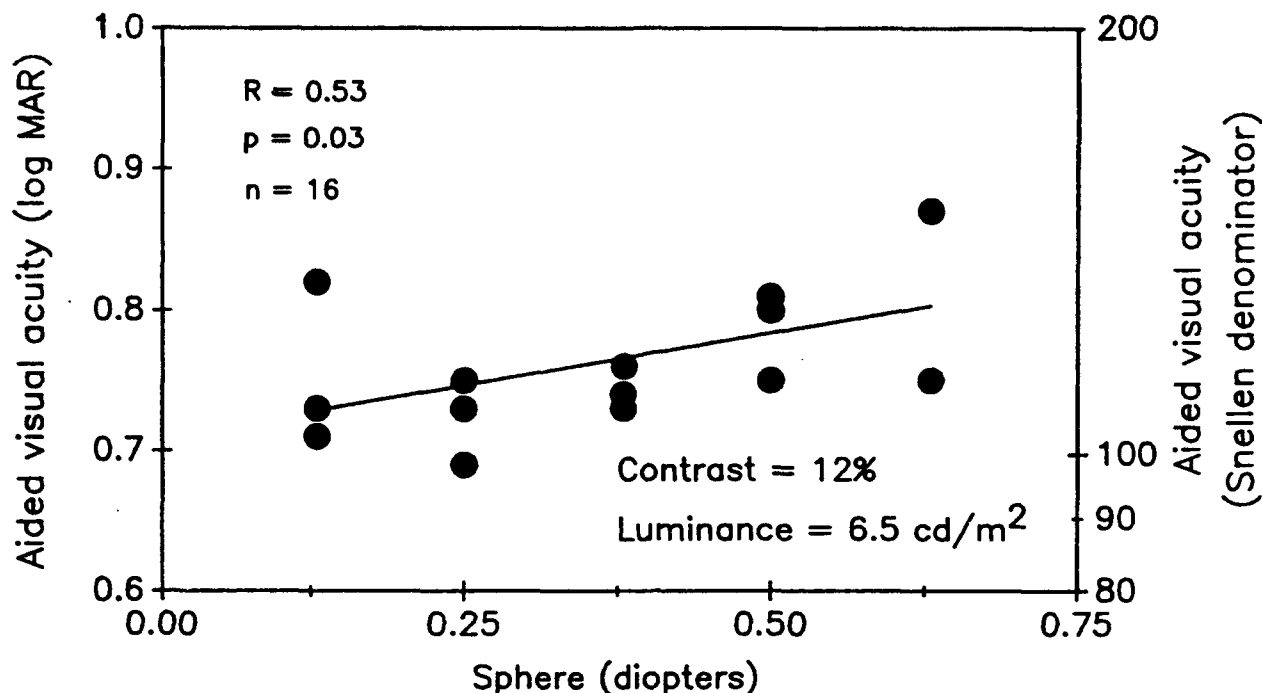


Figure 6. The relationship between uncorrected NVG VA and the absolute value of the spherical component of the refractive error for nominal emmetropes. The NVG eyepieces were focused to infinity.

reveals that aided VA is correlated with the power of the spherical component of the refractive error when target contrast is low and the instrument eyepieces are focused to infinity.

Figure 7 demonstrates that there is also a correlation between aided and unaided VA for emmetropes when the eyepieces are focused at infinity. This relationship is statistically significant at both high ($R = 0.73$, $p = 0.001$) and low ($R = 0.61$, $p = 0.01$) contrast. However, the relationship ceases to be significant when the focus is adjusted by the user for best vision ($R = 0.18$, $p = 0.5$ at high contrast; $R = 0.39$, $p = 0.13$ at low contrast).

Multivariate relationships

Multiple regression was used to predict aided VA by building a model which includes only those independent variables that add markedly to the strength of prediction. Tables 3 and 4 list the variables that were tested as potential predictors of aided VA for the fixed infinity focus condition, and Tables 5 and 6 list the variables that were tested for the adjustable focus

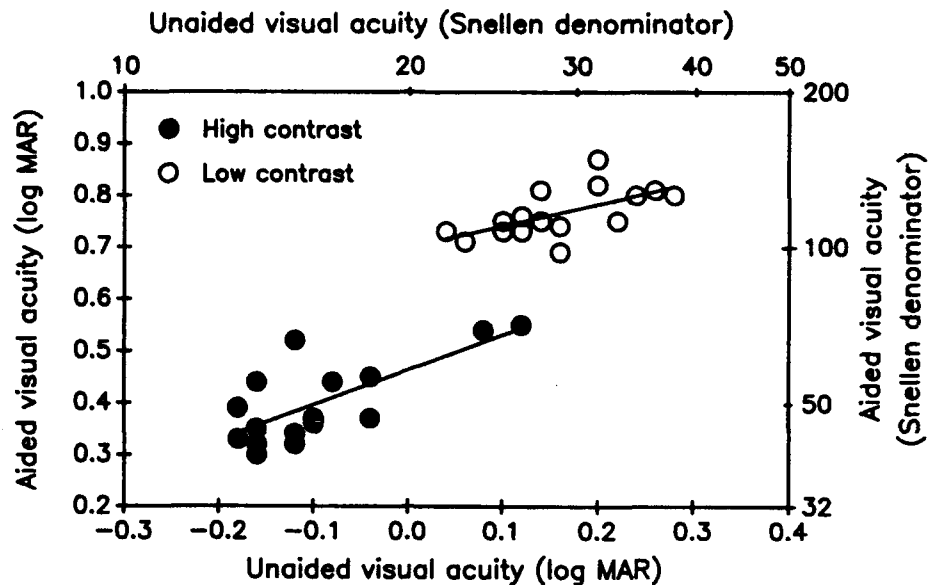


Figure 7. The relationship between uncorrected NVG VA and uncorrected unaided VA for nominal emmetropes. The NVG eyepieces were focused to infinity. Table 1 gives the values for high and low contrast for the aided and unaided VA measurements.

condition. In these tables, partial correlation is equivalent to Pearson's R in simple linear regression, and F-to-enter is the test statistic for determining whether R is significant.

Fixed infinity focus condition

Aided visual acuity for high contrast targets

The list of candidate independent variables to predict aided VA for high contrast targets is given in Table 3. The variables that were selected from this list are given by the equation below, in which A_A represents aided acuity, A_U represents unaided acuity (high contrast), and N_L represents the log of NVG flight hours (a log transform was performed because the distribution of NVG flight hours was asymmetric).

$$A_A = 0.50A_U - 0.08N_L + 0.58$$

The relative contribution of each independent variable to the model can be inferred from the percent of variance explained. Unaided VA, the most predictive variable (highest F-to-enter value in Table 3), alone explained 37 percent of the variance of

aided VA, i.e., $R^2 = 0.37$. The combination of unaided VA and log NVG hours explained 60 percent of the variance of aided VA, i.e., $R^2 = 0.60$. Thus, the addition of log NVG hours to the model increased the prediction of the dependent variable by 23 percent ($60 - 37 = 23$).

Table 3.
List of candidate independent variables to predict aided visual acuity (high contrast) when the eyepiece is focused at infinity.

Variable	Partial correlation	F-to-enter
Unaided VA	0.61	6.50
Equivalent sphere	0.49	3.45
Sphere	0.39	1.99
Cylinder	0.41	2.16
Flight hours	-0.32	1.25
Log flight hours	-0.38	1.84
NVG hours	-0.49	3.40
Log NVG hours	-0.59	5.97

Table 4.
List of candidate independent variables to predict aided visual acuity (low contrast) when the eyepiece is focused at infinity.

Variable	Partial correlation	F-to-enter
Unaided VA	0.60	6.04
Equivalent sphere	0.30	1.05
Sphere	0.42	2.14
Cylinder	0.53	4.30
Flight hours	-0.57	5.39
Log flight hours	-0.60	6.06
NVG hours	-0.36	1.60
Log NVG hours	-0.43	2.45

Table 5.
List of candidate independent variables
to predict aided visual acuity (high contrast)
when the eyepiece is focused for best vision.

Variable	Partial correlation	F-to-enter
Unaided VA	0.29	1.01
Equivalent sphere	0.17	0.33
Sphere	0.18	0.37
Cylinder	0.21	0.53
Flight hours	0.09	0.09
Log flight hours	0.06	0.04
NVG hours	-0.28	0.93
Log NVG hours	-0.32	1.26

Table 6.
List of candidate independent variables to predict
aided visual acuity (low contrast) when
the eyepiece is focused for best vision.

Variable	Partial correlation	F-to-enter
Unaided VA	0.34	1.43
Equivalent sphere	-0.09	0.08
Sphere	0.22	0.58
Cylinder	0.17	0.33
Flight hours	-0.20	0.46
Log flight hours	-0.11	0.14
NVG hours	-0.09	0.09
Log NVG hours	-0.11	0.14

Aided visual acuity for low contrast targets

The list of candidate independent variables to predict aided VA for low contrast targets is given in Table 4. The variables that were selected from this list are given by the equation below, in which A_A represents aided acuity, A_U represents unaided acuity, and F_L represents the common logarithm of total flight hours (a log transform was performed because the distribution of total flight hours was asymmetric).

$$A_A = -0.04F_L + 0.34A_U + 0.82$$

The most predictive variable was log flight hours (highest F-to-enter value in Table 4), which alone explained 36 percent of the variance of aided VA, i.e., $R^2 = 0.36$. The combination of log flight hours and unaided VA explained 53 percent of the variance of aided VA, i.e., $R^2 = 0.53$. Thus, the addition of unaided VA to the model increased the prediction of the dependent variable by 17 percent ($53 - 36 = 17$).

User adjusted focus aided condition

When the NVG focus was adjusted by the user for best vision, aided VA was not predictable by any of the candidate independent variables. This was true at both levels of contrast (Tables 5 and 6).

Discussion

We found that the between-subject variations in unaided VA of nominal emmetropes do manifest themselves as corresponding fluctuations in aided VA when the NVG eyepieces are focused at infinity. This effect is robust with respect to changes in target contrast. However, the effect diminishes significantly when the eyepieces are focused by the user for best vision. This suggests that the relationship between unaided and aided VA among emmetropes is mainly due to an optical factor, e.g., clinically insignificant refractive error.

Multiple regression revealed that, when the eyepieces were focused at infinity, unaided VA and experience as a visual observer (i.e., log NVG hours and log flight hours) were important determinants of NVG VA. At high contrast, unaided VA explained the greatest proportion of the variance of NVG VA. At low contrast, total flight hours explained the greatest proportion of the variance of NVG VA. This suggests that experience as a visual observer is more important under degraded

stimulus conditions than it is under optimal conditions. Refractive error was not selected for any of the multiple regression models although it is related to aided VA (Figure 6). This is because refractive error does not explain any of the variability of NVG VA that is not already explained by unaided VA.

Our data on the relationship between unaided and NVG VA among emmetropes is consistent with data from other studies in which the subjects had reduced unaided VA either due to astigmatism (Kim, 1982) or to eye disease (Hoover, 1983). The data from all three studies are fit well by the same regression line ($R = 0.87$) (Figure 8). Since there appears to be no significant difference between Kim's data from ametropes and Hoover's data from visually impaired subjects, perhaps the source of reduced unaided VA is not important in predicting aided VA.

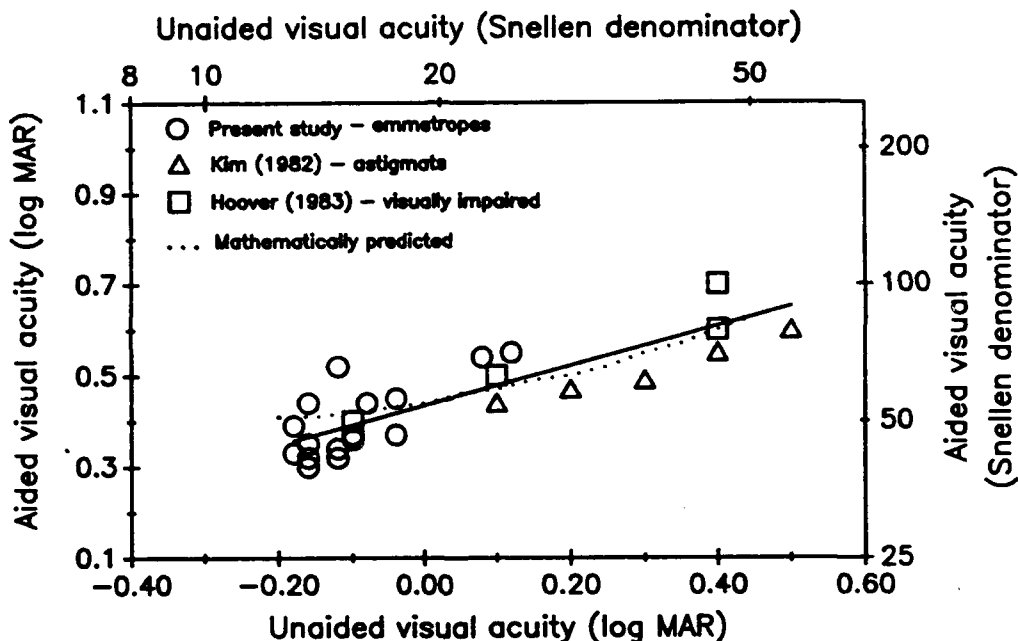


Figure 8. The relationship between NVG to unaided VAs, comparing observed to predicted results. A simple mathematical model seems to agree well with laboratory data from three independent studies.

Because Kim did not report unaided VA, we converted his measured astigmatism data to unaided VA based on the known relationship between the two (Peters, 1961). We controlled for between-study differences in NVG generation by comparing VAs from infinity focus third generation NVGs to VAs from adjustable focus second generation NVGs, because VAs have been shown to be similar under these two conditions (Kotulak and Morse, 1994a). In addition, we

modified the exponents of the equation described in the introduction (Farrell and Booth, 1984) to obtain a better fit of the data, i. e.,

$$\frac{1}{R_C^{1.6}} = \frac{1}{R_H^{1.6}} + \frac{1}{R_L^{1.6}}$$

As can be seen in Figure 8, the predictions based on the modified equation are in close agreement with the observed results. This suggests that the Farrell and Booth resolution model is applicable to the eye-NVG system with only minor modification. Additional work needs to be done to determine the relationship between NVG and unaided VA for subjects with unaided VAs beyond the range of Figure 8.

The military significance of the present work lies with night vision devices which are either not spectacle compatible or which have a fixed focus eyepiece. An example of the former is the full faceplate AN/PVS-5 NVG that is used for ground troops, and an example of the latter is the helmet mounted display that is under development for the Comanche helicopter. The AN/PVS-5 has adjustable focus eyepieces, which when set properly, compensate for spherical refractive error (i.e., simple myopia or hyperopia) but not for astigmatism. The Comanche helmet mounted display will be spectacle compatible, but will have eyepieces in which the focus is fixed at infinity. The results of this study, whether considered alone or with the works of Kim (1982) and Hoover (1983), suggest that for either type of device any decrement in unaided VA produces an analogous loss in NVG VA.

References

- Bailey, I. L. 1982. Simplifying contrast sensitivity testing. American journal of optometry and physiological optics. 59:12.
- Bailey, I. L., Bullimore, M. A., Raasch, T. W., and Taylor, H. R. 1991. Clinical grading and the effects of scaling. Investigative ophthalmology and visual science. 32:422-432.
- Bailey, I. L., and Lovie, J. E. 1976. New design principles for visual acuity letter charts. American journal of optometry and physiological optics. 53:740-745.
- Donohue-Perry, M. M., Riegler, J. T., and Hausman, M. A. 1990. A compatibility assessment of the protective integrated hood mask with ANVIS night vision goggles. Wright-Patterson Air Force Base, OH: Armstrong Aerospace Medical Research Laboratory. Report No. AAMRL-TR-90-030.
- Farrell, R. J., and Booth, J. M. 1984. Design handbook for imagery interpretation equipment. Seattle: Boeing Aerospace.
- Hirsch, M. J. 1945. Relation of visual acuity to myopia. Archives of ophthalmology. 34:418-421.
- Hoover, K. L. 1983. Visual acuity with the ITT night vision aid for patients with night blindness. American journal of optometry and physiological optics. 60:762-768.
- Jenkins, D., and Efkenan, A. 1980. Development of an aviator's night vision imaging system (ANVIS). In Optomechanical systems design, 18-23. SPIE Vol. 250. Bellingham, WA.
- Kim, H. J. 1982. Prevalence of astigmatism among aviators and its effect upon visual performance with the AN/PVS-5 night vision goggles. Paper presented at annual meeting of Aerospace Medical Association, 12 May, Bal Harbour, FL.
- King, J. M., and Morse, S. E. 1992. Interpupillary and vertex distance effects on field-of-view with ANVIS. Fort Rucker, AL: U.S. Army Aeromedical Research Laboratory. USAARL Report No. 93-9.
- Kotulak, J. C., and Morse, S. E. 1992. The effects of instrument myopia and user focus adjustments on visual acuity with optical instruments. Optometry and vision science supplement. 69:145.

- Kotulak, J. C., and Morse, S. E. 1994a. The effects of focus adjustment on visual acuity and oculomotor balance with aviator night vision displays. Aviation, space and environmental medicine. 65:348-352.
- Kotulak, J. C., and Morse, S. E. 1994b. The relationship between accommodation, focus, and resolution with optical instruments. Journal of the optical society of America A. 11:71-79.
- Kotulak, J. C., Morse, S. E., and Wiley, R. W. 1994. The effect of knowledge of object distance on accommodation during instrument viewing. Perception. In press.
- Kotulak, J. C., and Rash, C. E. 1992. Visual acuity with second and third generation night vision goggles, obtained with a new method of night sky simulation, across a wide range of target contrast. Fort Rucker, AL: U.S. Army Aeromedical Research Laboratory. USAARL Report No. 92-9.
- Levine, R. R., and Rash, C. E. 1989a. Visual acuity with AN/PVS-5A night vision goggles and simulated flashblindness protective lenses under varying levels of brightness and contrast. Fort Rucker, AL: U.S. Army Aeromedical Research Laboratory. USAARL Report No. 89-16.
- Levine, R. R., and Rash, C. E. 1989b. Attenuating the luminous output of the AN/PVS-5A night vision goggles and its effects on visual acuity. Fort Rucker, AL: U.S. Army Aeromedical Research Laboratory. USAARL Report No. 89-24.
- Lovie-Kitchin, J. E. 1988. Validity and reliability of visual acuity measurements. Ophthalmic and physiological optics. 8:363-370.
- Miller, R. E., II, Provines, W. F., Block, M. G., Miller, J. M., and Tredici, T. J. 1984. Comparative visual performance with ANVIS and AN/PVS-5A night vision goggles under starlight conditions. Brooks Air Force Base, TX: U.S. Air Force School of Aerospace Medicine. Report No. USAFSAM-TR-84-28.
- Miller, R. E., Woessner, W. M., Wooley, L. M., Dennis, R. J., and Green, R. P. 1989. Compatibility of night vision goggles and chemical warfare masks. Brooks Air Force Base, TX: U.S. Air Force School of Aerospace Medicine. Report No. USAFSAM-TR-89-3.
- Miwa, T. 1992. Instrument myopia and the resting state of accommodation. Optometry and vision science. 69:55-59.

- National Research Council. 1979. Recommended standard procedures for the clinical measurement and specification of visual acuity. Washington, DC: Committee on Vision, National Academy of Science.
- Peters, H. B. 1961. The relationship between refractive error and visual acuity at three age levels. American journal of optometry and physiological optics. 38:194-198.
- Riegler, J. T., Whiteley, J. D., Task, H. L., and Schueren, J. 1991. The effect of signal-to-noise ratio on visual acuity through night vision goggles. Wright-Patterson Air Force Base, OH: Armstrong Laboratory. Report No. AL-TR-91-0011.
- Sheedy, J. E., Bailey, I. L., and Raasch, T. W. 1984. Visual acuity and chart luminance. American journal of optometry and physiological optics. 61:595-600.
- Wiley, R. W. 1989. Visual acuity and stereopsis with night vision goggles. Fort Rucker, AL: U.S. Army Aeromedical Research Laboratory. USAARL Report No. 89-9.

Initial distribution

Commander, U.S. Army Natick Research,
Development and Engineering Center
ATTN: SATNC-MIL (Documents
Librarian)
Natick, MA 01760-5040

U.S. Army Communications-Electronics
Command
ATTN: AMSEL-RD-ESA-D
Fort Monmouth, NJ 07703

Commander
10th Medical Laboratory
ATTN: Audiologist
APO New York 09180

Naval Air Development Center
Technical Information Division
Technical Support Detachment
Warminster, PA 18974

Commanding Officer, Naval Medical
Research and Development Command
National Naval Medical Center
Bethesda, MD 20814-5044

Deputy Director, Defense Research
and Engineering
ATTN: Military Assistant
for Medical and Life Sciences
Washington, DC 20301-3080

Commander, U.S. Army Research
Institute of Environmental Medicine
Natick, MA 01760

Library
Naval Submarine Medical Research Lab
Box 900, Naval Sub Base
Groton, CT 06349-5900

Director, U.S. Army Human
Engineering Laboratory
ATTN: Technical Library
Aberdeen Proving Ground, MD 21005

Commander
Man-Machine Integration System
Code 602
Naval Air Development Center
Warminster, PA 18974

Commander
Naval Air Development Center
ATTN: Code 602-B (Mr. Brindle)
Warminster, PA 18974

Commanding Officer
Armstrong Laboratory
Wright-Patterson
Air Force Base, OH 45433-6573

Director
Army Audiology and Speech Center
Walter Reed Army Medical Center
Washington, DC 20307-5001

Commander/Director
U.S. Army Combat Surveillance
and Target Acquisition Lab
ATTN: SFAE-IEW-JS
Fort Monmouth, NJ 07703-5305

Commander, U.S. Army Institute
of Dental Research
ATTN: Jean A. Setterstrom, Ph. D.
Walter Reed Army Medical Center
Washington, DC 20307-5300

Commander, U.S. Army Test
and Evaluation Command
ATTN: AMSTE-AD-H
Aberdeen Proving Ground, MD 21005

Naval Air Systems Command
Technical Air Library 950D
Room 278, Jefferson Plaza II
Department of the Navy
Washington, DC 20361

Director
U.S. Army Ballistic
Research Laboratory
ATTN: DRXBR-OD-ST Tech Reports
Aberdeen Proving Ground, MD 21005

Commander
U.S. Army Medical Research
Institute of Chemical Defense
ATTN: SGRD-UV-AO
Aberdeen Proving Ground,
MD 21010-5425

Commander, U.S. Army Medical
Research and Development Command
ATTN: SGRD-RMS (Ms. Madigan)
Fort Detrick, Frederick, MD 21702-5012

Director
Walter Reed Army Institute of Research
Washington, DC 20307-5100

HQ DA (DASG-PSP-O)
5109 Leesburg Pike
Falls Church, VA 22041-3258

Harry Diamond Laboratories
ATTN: Technical Information Branch
2800 Powder Mill Road
Adelphi, MD 20783-1197

U.S. Army Materiel Systems
Analysis Agency
ATTN: AMXSY-PA (Reports Processing)
Aberdeen Proving Ground
MD 21005-5071

U.S. Army Ordnance Center
and School Library
Simpson Hall, Building 3071
Aberdeen Proving Ground, MD 21005

U.S. Army Environmental
Hygiene Agency
ATTN: HSHB-MO-A
Aberdeen Proving Ground, MD 21010

Technical Library Chemical Research
and Development Center
Aberdeen Proving Ground, MD
21010-5423

Commander
U.S. Army Medical Research
Institute of Infectious Disease
SGRD-UIZ-C
Fort Detrick, Frederick, MD 21702

Director, Biological
Sciences Division
Office of Naval Research
600 North Quincy Street
Arlington, VA 22217

Commander
U.S. Army Materiel Command
ATTN: AMCDE-XS
5001 Eisenhower Avenue
Alexandria, VA 22333

Commandant
U.S. Army Aviation
Logistics School ATTN: ATSQ-TDN
Fort Eustis, VA 23604

Headquarters (ATMD)
U.S. Army Training
and Doctrine Command
ATTN: ATBO-M
Fort Monroe, VA 23651

IAF Liaison Officer for Safety
USAF Safety Agency/SEFF
9750 Avenue G, SE
Kirtland Air Force Base
NM 87117-5671

Naval Aerospace Medical
Institute Library
Building 1953, Code 03L
Pensacola, FL 32508-5600

Command Surgeon
HQ USCENTCOM (CCSG)
U.S. Central Command
MacDill Air Force Base, FL 33608

Air University Library
(AUL/LSE)
Maxwell Air Force Base, AL 36112

U.S. Air Force Institute
of Technology (AFIT/LDEE)
Building 640, Area B
Wright-Patterson
Air Force Base, OH 45433

Henry L. Taylor
Director, Institute of Aviation
University of Illinois-Willard Airport
Savoy, IL 61874

Chief, National Guard Bureau
ATTN: NGB-ARS (COL Urbauer)
Room 410, Park Center 4
4501 Ford Avenue
Alexandria, VA 22302-1451

Commander
U.S. Army Aviation Systems Command
ATTN: SGRD-UAX-AL
4300 Goodfellow Blvd., Building 105
St. Louis, MO 63120

U.S. Army Aviation Systems Command
Library and Information Center Branch
ATTN: AMSAV-DIL
4300 Goodfellow Boulevard
St. Louis, MO 63120

Federal Aviation Administration
Civil Aeromedical Institute
Library AAM-400A
P.O. Box 25082
Oklahoma City, OK 73125

Commander
U.S. Army Academy
of Health Sciences
ATTN: Library
Fort Sam Houston, TX 78234

Commander
U.S. Army Institute of Surgical Research
ATTN: SGRD-USM (Jan Duke)
Fort Sam Houston, TX 78234-6200

AAMRL/HEX
Wright-Patterson
Air Force Base, OH 45433

John A. Dellinger,
Southwest Research Institute
P. O. Box 28510
San Antonio, TX 78284

Product Manager
Aviation Life Support Equipment
ATTN: AMCPM-ALSE
4300 Goodfellow Boulevard
St. Louis, MO 63120-1798

Commander and Director
USAE Waterways Experiment Station
ATTN: CEWES-IM-MI-R

Alfrieda S. Clark, CD Department
3909 Halls Ferry Road
Vicksburg, MS 39180-6199

Commanding Officer
Naval Biodynamics Laboratory
P.O. Box 24907
New Orleans, LA 70189-0407

Assistant Commandant
U.S. Army Field Artillery School
ATTN: Morris Swott Technical Library
Fort Sill, OK 73503-0312

Mr. Peter Seib
Human Engineering Crew Station
Box 266
Westland Helicopters Limited
Yeovil, Somerset BA20 2YB UK

U.S. Army Dugway Proving Ground
Technical Library, Building 5330
Dugway, UT 84022

U.S. Army Yuma Proving Ground
Technical Library
Yuma, AZ 85364

AFFTC Technical Library
6510 TW/TSTL
Edwards Air Force Base,
CA 93523-5000

Commander
Code 3431
Naval Weapons Center
China Lake, CA 93555

Aeromechanics Laboratory
U.S. Army Research and Technical Labs
Ames Research Center, M/S 215-1
Moffett Field, CA 94035

Sixth U.S. Army
ATTN: SMA
Presidio of San Francisco, CA 94129

Commander
U.S. Army Aeromedical Center
Fort Rucker, AL 36362

Strughold Aeromedical Library
Document Service Section
2511 Kennedy Circle
Brooks Air Force Base, TX 78235-5122

Dr. Diane Damos
Department of Human Factors
ISSM, USC
Los Angeles, CA 90089-0021

U.S. Army White Sands
Missile Range
ATTN: STEWS-IM-ST
White Sands Missile Range, NM 88002

U.S. Army Aviation Engineering
Flight Activity
ATTN: SAVTE-M (Tech Lib) Stop 217
Edwards Air Force Base, CA 93523-5000

Ms. Sandra G. Hart
Ames Research Center
MS 262-3
Moffett Field, CA 94035

Commander, Letterman Army Institute
of Research
ATTN: Medical Research Library
Presidio of San Francisco, CA 94129

Commander
U.S. Army Medical Materiel
Development Activity
Fort Detrick, Frederick, MD 21702-5009

Commander
U.S. Army Health Services Command
ATTN: HSOP-SO
Fort Sam Houston, TX 78234-6000

U. S. Army Research Institute
Aviation R&D Activity
ATTN: PERI-IR
Fort Rucker, AL 36362

Commander
U.S. Army Safety Center
Fort Rucker, AL 36362

U.S. Army Aircraft Development
Test Activity
ATTN: STEBG-MP-P
Cairns Army Air Field
Fort Rucker, AL 36362

Commander, U.S. Army Medical Research
and Development Command
ATTN: SGRD-PLC (COL Schnakenberg)
Fort Detrick, Frederick, MD 21702

TRADOC Aviation LO
Unit 21551, Box A-209-A
APO AE 09777

Netherlands Army Liaison Office
Building 602
Fort Rucker, AL 36362

British Army Liaison Office
Building 602
Fort Rucker, AL 36362

Italian Army Liaison Office
Building 602
Fort Rucker, AL 36362

Directorate of Training Development
Building 502
Fort Rucker, AL 36362

Chief
USAHEL/USAAVNC Field Office
P. O. Box 716
Fort Rucker, AL 36362-5349

Commander, U.S. Army Aviation Center
and Fort Rucker
ATTN: ATZQ-CG
Fort Rucker, AL 36362

Chief
Test & Evaluation Coordinating Board
Cairns Army Air Field
Fort Rucker, AL 36362

MAJ Terry Newman
Canadian Army Liaison Office
Building 602
Fort Rucker, AL 36362

German Army Liaison Office
Building 602
Fort Rucker, AL 36362

French Army Liaison Office
USAAVNC (Building 602)
Fort Rucker, AL 36362-5021

Australian Army Liaison Office
Building 602
Fort Rucker, AL 36362

Dr. Garrison Rapmund
6 Burning Tree Court
Bethesda, MD 20817

Commandant, Royal Air Force
Institute of Aviation Medicine
Farnborough, Hampshire GU14 6SZ UK

Commander
U.S. Army Biomedical Research
and Development Laboratory
ATTN: SGRD-UBZ-I
Fort Detrick, Frederick, MD 21702

Defense Technical Information
Cameron Station, Building 5
Alexandra, VA 22304-6145

Commander, U.S. Army Foreign Science
and Technology Center
AIFRTA (Davis)
220 7th Street, NE
Charlottesville, VA 22901-5396

Director,
Applied Technology Laboratory
USARTL-AVSCOM
ATTN: Library, Building 401
Fort Eustis, VA 23604

Commander, U.S. Air Force
Development Test Center
101 West D Avenue, Suite 117
Eglin Air Force Base, FL 32542-5495

Aviation Medicine Clinic
TMC #22, SAAF
Fort Bragg, NC 28305

Dr. H. Dix Christensen
Bio-Medical Science Building, Room 753
Post Office Box 26901
Oklahoma City, OK 73190

Commander, U.S. Army Missile
Command
Redstone Scientific Information Center
ATTN: AMSMI-RD-CS-R
/ILL Documents
Redstone Arsenal, AL 35898

Director
Army Personnel Research Establishment
Farnborough, Hants GU14 6SZ UK

U.S. Army Research and Technology
Laboratories (AVSCOM)
Propulsion Laboratory MS 302-2
NASA Lewis Research Center
Cleveland, OH 44135

COL John F. Glenn
U.S. Army Medical Research
& Development Command
SGRD-ZC
Fort Detrick, Frederick, MD 21702-5012

Dr. Eugene S. Channing
166 Baughman's Lane
Frederick, MD 21702-4083

USAMRDC Liaison at Academy
of Health Sciences
ATTN: HSHA-ZAC-F
Fort Sam Houston, TX 78234

Dr. A. Kornfield, President
Biosearch Company
3016 Revere Road
Drexel Hill, PA 29026

NVESD
AMSEL-RD-NV-ASID-PST
(Attn: Trang Bui)
10221 Burbeck Road
Fort Belvoir, VA 22060-5806

CA Av Med
HQ DAAC
Middle Wallop
Stockbridge, Hants S020 8DY UK

Dr. Christine Schlichting
Behavioral Sciences Department
Box 900, NAVUBASE NLON
Groton, CT 06349-5900

Commander, HQ AAC/SGPA
Aerospace Medicine Branch
ATTN: CPT Joseph R. Smith
162 Dodd Boulevard, Suite 100
Langley Air Force Base,
VA 23665-1995

COL C. Fred Tyner
U.S. Army Medical Research
& Development Command
SGRD-ZB
Fort Detrick, Frederick, MD 21702-5012

Director
Directorate of Combat Developments
ATZQ-CD
Building 515
Fort Rucker, AL 36362